



Tibia & Fibula

stryker®

AxSOS

Locking Plate System

Operative Technique

- Proximal Lateral Tibia
- Alternating threaded shaft holes

Tibia Fractures



This publication sets forth detailed recommended procedures for using Stryker Osteosynthesis devices and instruments.

It offers guidance that you should heed, but, as with any such technical guide, each surgeon must consider the particular needs of each patient and make appropriate adjustments when and as required.

A workshop training is recommended prior to first surgery.

All non-sterile devices must be cleaned and sterilized before use. Follow the instructions provided in our reprocessing guide (L24002000). Multi-component instruments must be disassembled for cleaning. Please refer to the corresponding assembly/disassembly instructions.

See package insert (V15011 and V15013) for a complete list of potential adverse effects, contraindications, warnings and precautions. The surgeon must discuss all relevant risks, including the finite lifetime of the device, with the patient, when necessary.

Warning:

Fixation Screws:
Stryker Osteosynthesis bone screws are not approved or intended for screw attachment or fixation to the posterior elements (pedicles) of the cervical, thoracic or lumbar spine.

Contents

	Page
1. Introduction	4
2. Features & Benefits	5
3. Indications, Precautions & Contraindications	6
Indications	6
Precautions	6
Contraindications	6
4. Operative Technique	7
General Guidelines	7
Step 1 – Pre-Operative Planning	9
Step 2 – Pre-Operative Locking Insert Application	9
Step 2a – Locking Insert Extraction	10
Step 2b – Intra-Operative Locking Insert Application	10
Step 3 – Aiming Block/Plate Insertion Handle Assembly	11
Step 4 – Plate Application	11
Step 5 – Primary Plate Fixation Proximal	12
Step 6 – Primary Plate Fixation – Distal (Optional)	13
Step 7 – Metaphyseal Locking	13
Step 8 – Shaft Fixation	15
Option 1 – Standard Screws	15
Option 2 – Locking Screws	16
Step 9 - Kick-Stand Screw Placement	16
Sub-Muscular Insertion Technique	17
5. Additional Tips	19
<hr/>	
Ordering Information – Implants	20
Ordering Information – Instruments	22
Ordering Information – Instruments	24
Additional Information – HydroSet Injectable HA	25
Indications	25
Advantages	25

Introduction

The AxSOS Locking Plate System is intended for use in long bone fracture fixation. The AxSOS Locking Plate System is indicated for fixation of long bone fractures including fractures of the distal radius, the proximal humerus, the distal tibia, proximal tibia and the distal femur.

The system design is based on clinical input from an international panel of experienced surgeons, data from literature, and both practical and biomechanical testing.

The anatomical shape, the fixed screw trajectory, and high surface quality take into account the current demands of clinical physicians for appropriate fixation, high fatigue strength, and minimal soft tissue damage.

This Operative Technique contains a simple step-by-step procedure for the implantation of the Proximal Lateral Tibial Plate.


Proximal Lateral Tibial Plate



Proximal Humeral Plate



Distal Lateral Femoral Plate

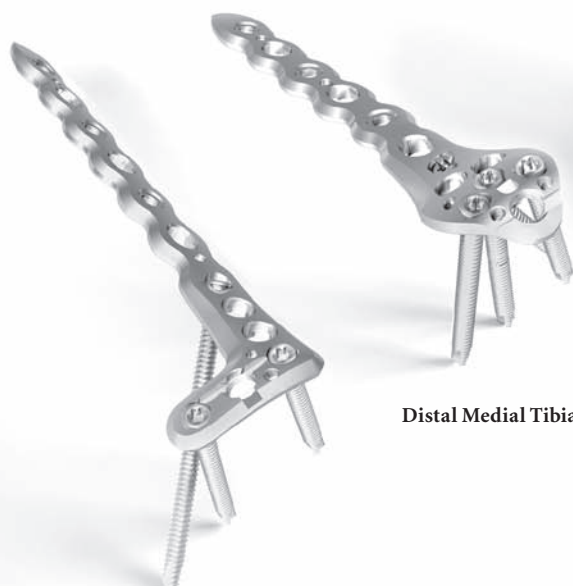

Distal Medial Tibial Plate

Distal Anterolateral Tibial Plate

Features & Benefits

System

The Proximal Lateral Tibial Plate is designed with divergent fixed-angled screw trajectories in the metaphyseal part and perpendicular fixed-angled screw trajectories in the diaphyseal part, which provide increased biomechanical stability. This helps prevent loss of reduction.

Instruments

- Simple technique, easy instrumentation with minimal components.
- Compatible with MIPO (Minimally Invasive Plate Osteosynthesis) technique using state of the art instrumentation.

Range

Longer plates cover a wider range of fractures.

5 Monoaxial holes

Allow axially stable screw placement, bringing stability to construct.

K-Wire/Reduction/Suture holes

- Primary/temporary plate and fracture fixation.
- Anchor point for soft tissue re-attachment.

Anatomically contoured

- Little or no bending required.
- May reduce OR time.
- Facilitates/allows for better soft tissue coverage.

Innovative Locking Screw design

- Screw is guided into plate.
- The single thread screw design allows easy insertion into the plate, reducing any potential for cross threading and cold welding.



'Waisted' plate shape

Uniform load transfer.

Rounded & Tapered Plate End

Helps facilitate sliding of plates sub-muscularly.

Aiming Block

- Facilitates the placement of the Drill Sleeve.
- Provides attachment point for Plate Insertion Handle.



Unthreaded Freedom Holes

- Freehand placement of screws.
- Lag Screw possibility.

Kick-Stand Screw

Aimed at posterior/medial fragment to provide strong triangular fixation.

Shaft Holes - Standard or Locking

- Compression, neutral or buttress fixation.
- Accept standard 3.5/4.0mm SPS screws.
- Accept Locking Insert for axially stable screws.
- Pre-drilled Locking Holes allow axially stable screw placement.



Indications, Precautions & Contraindications

Indications

The indication for use of this internal fixation device includes metaphyseal extra and intra articular fractures of the proximal Tibia.

Precautions

Stryker Osteosynthesis systems have not been evaluated for safety and compatibility in MR environment and have not been tested for heating or migration in the MR environment, unless specified otherwise in the product labeling or respective operative technique.

Contraindications

The physician's education, training and professional judgement must be relied upon to choose the most appropriate device and treatment. Conditions presenting an increased risk of failure include:

- Any active or suspected latent infection or marked local inflammation in or about the affected area.
- Compromised vascularity that would inhibit adequate blood supply to the fracture or the operative site.
- Bone stock compromised by disease, infection or prior implantation that can not provide adequate support and/or fixation of the devices.
- Material sensitivity, documented or suspected.
- Obesity. An overweight or obese patient can produce loads on the implant that can lead to failure of the fixation of the device or to failure of the device itself.
- Patients having inadequate tissue coverage over the operative site.

- Implant utilisation that would interfere with anatomical structures or physiological performance.
- Any mental or neuromuscular disorder which would create an unacceptable risk of fixation failure or complications in postoperative care.
- Other medical or surgical conditions which would preclude the potential benefit of surgery.

Detailed information is included in the instructions for use being attached to every implant.

See package insert for a complete list of potential adverse effects and contraindications. The surgeon must discuss all relevant risks, including the finite lifetime of the device, with the patient, when necessary.

Caution:

Bone Screws are not intended for screw attachment or fixation to the posterior elements (pedicles) of the cervical, thoracic or lumbar spine.

Operative Technique

General Guidelines

Patient Positioning:

Supine with option to flex the knee. Visualisation of the proximal tibia under Fluoroscopy in both the lateral and AP views is necessary.

Surgical Approach:

Lateral Parapatellar

Instrument / Screw Set:

4.0mm

Reduction

Anatomical reduction of the fracture should be performed either by direct visualisation with the help of percutaneous clamps, or alternatively a bridging external fixator can aid indirect reduction. Fracture reduction of the articular surface should be confirmed by direct vision, or fluoroscopy. Use K-Wires as necessary to temporarily secure the reduction.

Typically, K-Wires set parallel to the joint axis will not only act to hold and support the reduction, but also help to visualise/identify the joint. Care must be taken that these do not interfere with the required plate and screw positions.

Consideration must also be taken when positioning independent Lag Screws prior to plate placement to ensure that they do not interfere with the planned plate location or Locking Screw trajectories.

If any large bony defects are present they should be filled by either bone graft or bone substitute material.


Note:

When using a sub muscular technique, please refer to the relevant section on page 17.

Bending

In most cases, the pre-contoured plate will fit without the need for further bending. However, should additional bending of the plate be required (generally at the junction from the metaphysis to the shaft) the Bending Irons (REF 702756) should be used. Bending of the plate in the region of the metaphyseal locking holes will affect the ability to correctly seat the Locking Screws into the plate and is therefore not permitted.

Plate contouring in the shaft region below the oblong hole is not recommended. Plate contouring will affect the ability to place a Locking Insert into the shaft holes adjacent to the bending point.

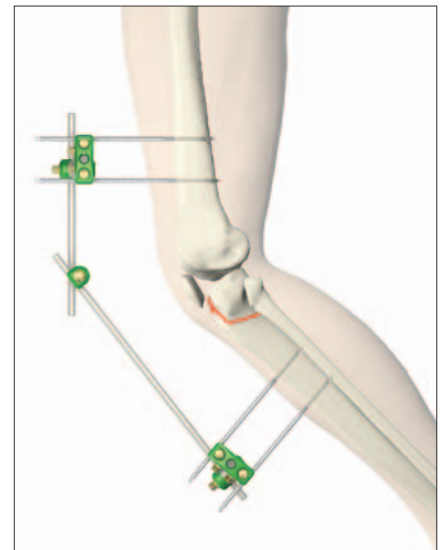

Operative Technique

General Guidelines

Locking Screw Measurement

There are four options to obtain the proper Locking Screw length as illustrated below.


Correct Screw Selection

Note:


Select a screw approximately 2-3mm shorter than the measured length to avoid screw penetrations through the opposite cortex in metaphyseal fixation.

Add 2-3mm to measured length for optimal bi-cortical shaft fixation.


Measurement Options

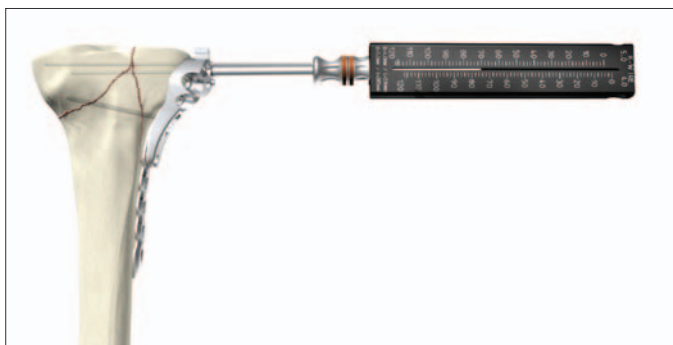


Measure off K-Wire

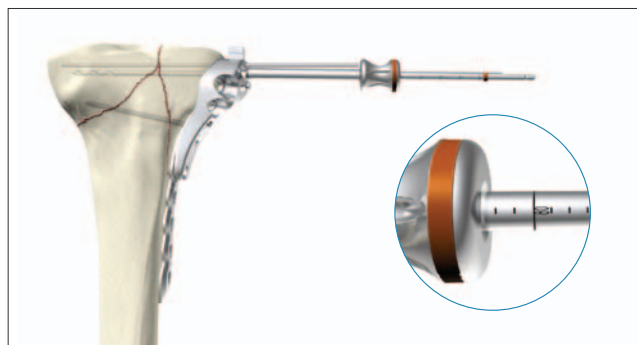

Read off drill bit calibration

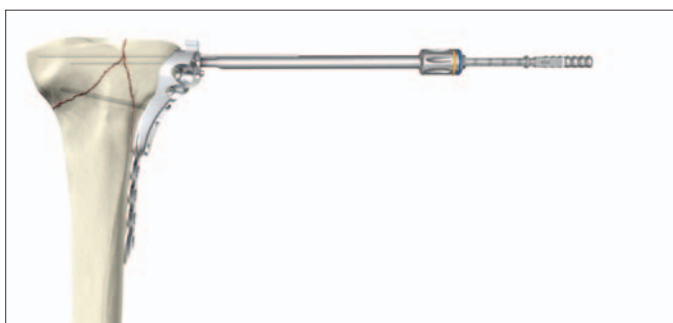

Conventional direct measurement

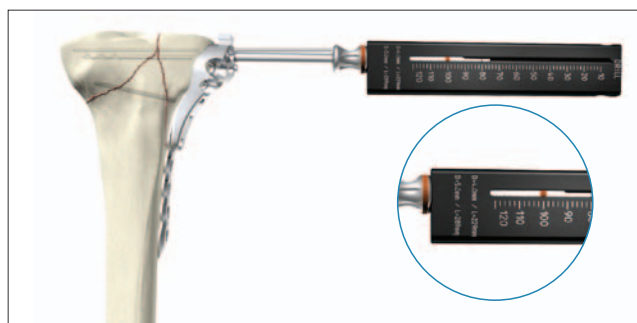

Measure off the end of drill bit

Soft-Tissue Reattachment

Special undercuts on the reverse side of the plate correlating to the two proximal K-Wire holes allows simple passing of sutures for meniscus reattachment after final plate fixation.



Operative Technique

Step 1 – Pre-Operative Planning

Use of the X-Ray Template (REF 981081) or Plate Trial (REF 702793) in association with fluoroscopy can assist in the selection of an appropriately sized implant (Fig. 1 & 1A).

If the Plate Trial is more than 90mm away from the bone, e.g. with obese patients, a magnification factor of 10-15% will occur and must be compensated for. Final intraoperative verification should be made to ensure correct implant selection.



Fig. 1

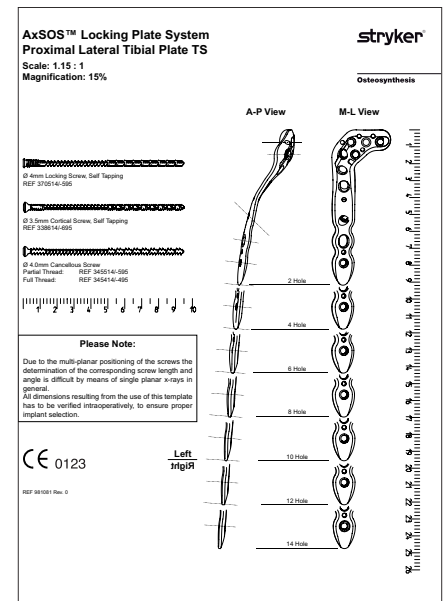


Fig. 1A

Step 2 – Pre-Operative Locking Insert Application

If additional Locking Screws are chosen for the plate shaft, pre-operative insertion of Locking Inserts is recommended.

A 4.0mm Locking Insert (REF 370002) is attached to the Locking Insert Insertor (REF 702762) and placed into the chosen holes in the shaft portion of the plate (Fig. 2). Ensure that the Locking Insert is properly placed. The Insertor should then be removed (Fig. 2A).

Note:

Do not place Locking Inserts with the Drill Sleeve.

It is important to note that if a Temporary Plate Holder is to be used for primary distal plate fixation, then a Locking Insert should not be placed in the same hole as the Temporary Plate Holder (See Step 6).

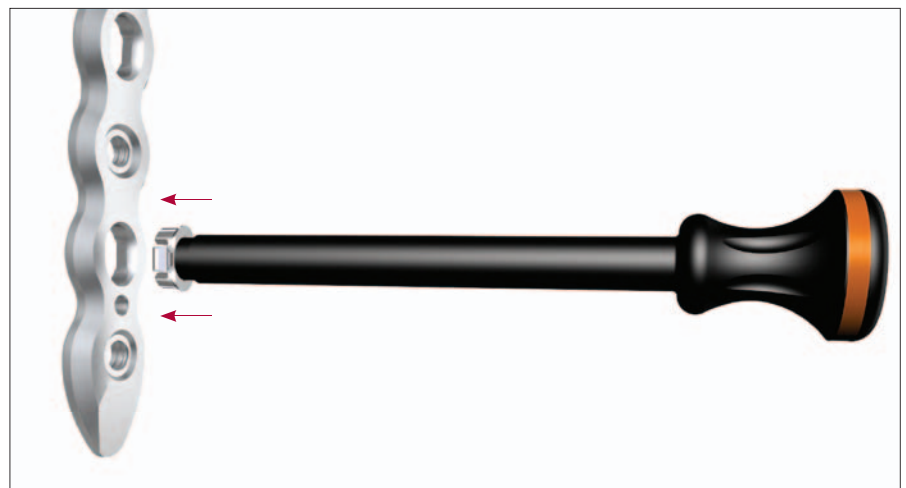


Fig. 2

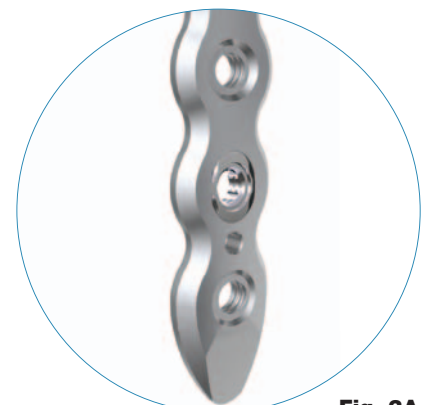


Fig. 2A

Operative Technique

Step 2a – Locking Insert Extraction

Should removal of a Locking Insert be required for any reason, then the following procedure should be used.

Thread the central portion (A) of the Locking Insert Extractor (REF 702767) into the Locking Insert that you wish to remove until it is fully seated (Fig. 2B).

Then turn the outer sleeve/collet (B) clockwise until it pulls the Locking Insert out of the plate. The Locking Insert must then be discarded, as it should not be reused (Fig. 2C).

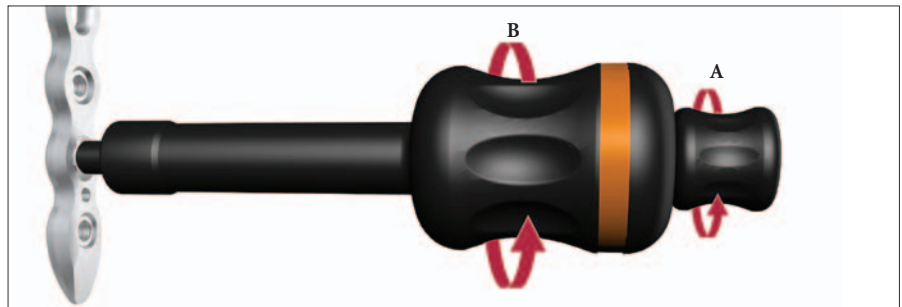


Fig. 2B

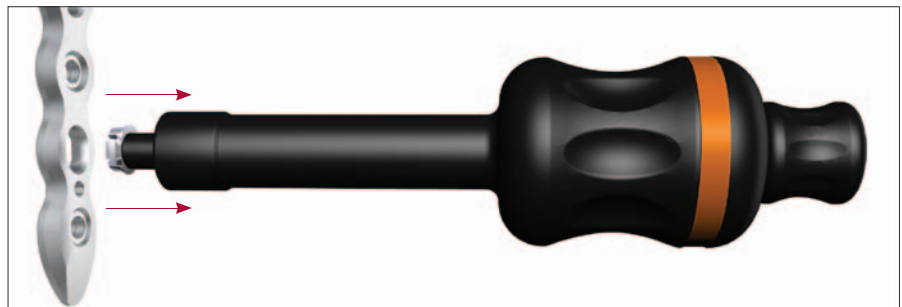


Fig. 2C

Step 2b – Intra-Operative Locking Insert Application

If desired, a Locking Insert can be applied in a standard hole in the shaft of the plate intra-operatively by using the Locking Insert Forceps (REF 702968), Centering Pin (REF 702673), Adaptor for Centering Pin (REF 702675), and Guide for Centering Pin (REF 702671).

First, the Centering Pin is inserted through the chosen hole using the Adaptor and Guide (Fig. 3A). It is important to use the Guide as this centers the core hole for Locking Screw insertion after the Locking Insert is applied. After inserting the Centering Pin bi-cortically, remove the Adaptor and Guide.

Next, place a Locking Insert on the end of the Forceps and slide the instrument over the Centering Pin down to the hole.

Last, apply the Locking Insert by triggering the forceps handle. Push the button on the Forceps to remove the device. At this time, remove the Centering Pin (Fig. 3B).



Fig. 3A

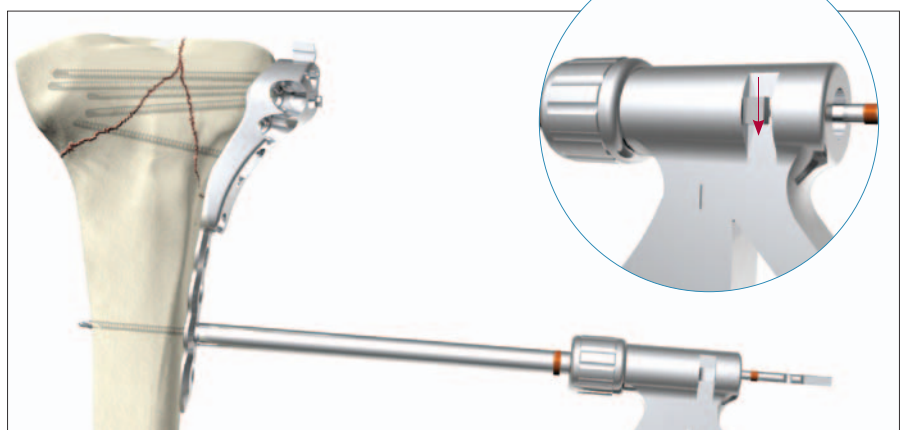


Fig. 3B

Operative Technique

Step 3 – Aiming Block/Plate Insertion Handle Assembly

Screw the appropriate Aiming Block (REF 702728/702729) to the plate using the Screwdriver T15 (REF 702747).

If desired, the Handle for Plate Insertion (REF 702778) can now be attached to help facilitate plate positioning and sliding of longer plates sub-muscularly (Fig. 4).

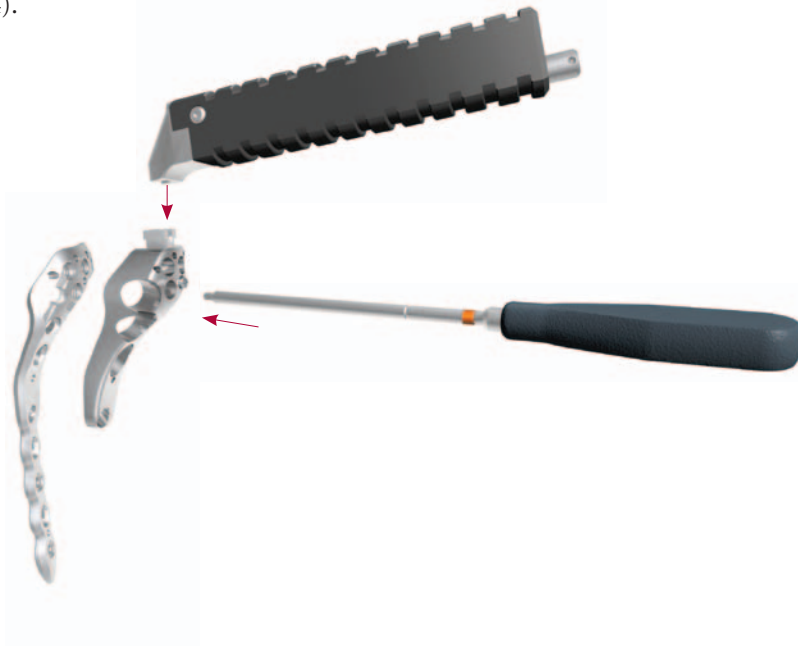


Fig. 4

Step 4 – Plate Application

After skin incision and anatomical reduction is achieved, apply the plate so that the lateral condyle is supported, with the proximal end of the plate approximately 5mm below the articular surface (Fig. 5).

This helps to ensure that the most proximal Locking Screws are directly supporting the joint surface.

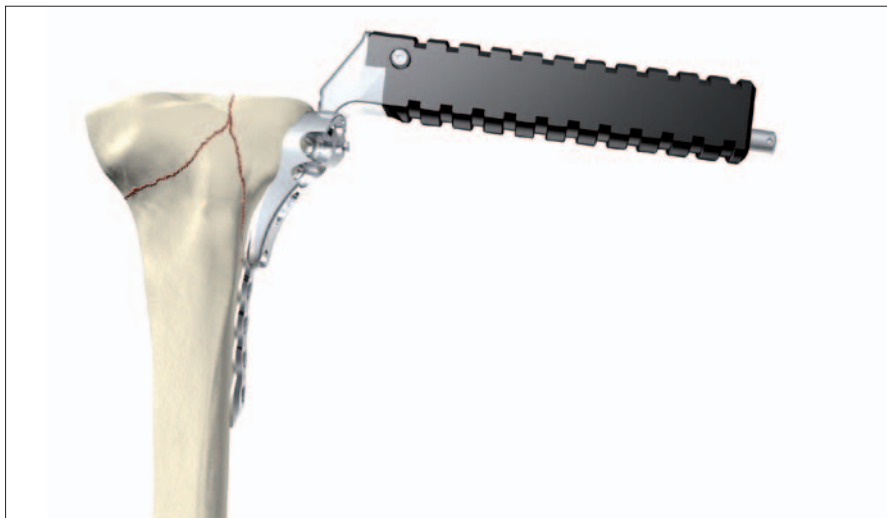


Fig. 5 – AP View

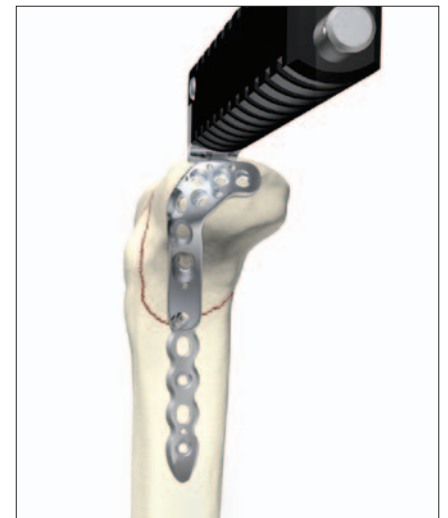


Fig. 5 – Lateral View

Operative Technique

Step 5 – Primary Plate Fixation Proximal

The K-Wire hole just distal to the oblong hole allows temporary plate fixation in the metaphysis (Fig. 6).

Using the K-Wire Sleeve (REF 702702) in conjunction with the Drill Sleeve (REF 702707), a 2.0×230mm K-Wire can then be inserted into the most posterior Locking Screw hole (Fig. 7).

This step shows the position of a posterior screw and also shows its relation to the joint surface. It will also confirm the screw will not be placed intra-articularly or too posterior exiting the cortex into the popliteal space.

Using fluoroscopy, the position of this K-Wire can be checked until the optimal position is achieved and the plate is correctly positioned. Correct distal placement should also be re-confirmed at this point to make sure the plate shaft is properly aligned over the lateral surface of the tibial shaft (Fig. 6).

If the proximal and axial alignment of the plate cannot be achieved, the K-Wires should be removed, the plate readjusted, and the above procedure repeated until both the posterior K-Wire and the plate are in the desired position.

Additional 2.0×150mm (REF 390192) K-Wires can be inserted in the K-Wire holes superior to the locking holes to further help secure the plate to the bone and also support depressed areas in fragments of the articular surface.

Do not remove the Drill Sleeve and K-Wire Sleeve at this point as it will cause a loss of the plate position.

Remove the Handle for Insertion by pressing the metal button at the end of the Handle.

Using a 2.5mm Drill (REF 700355 -230mm or 700347- 125mm) and Double Drill Guide (REF 702418), drill a core hole to the appropriate depth in the oblong hole of the plate.

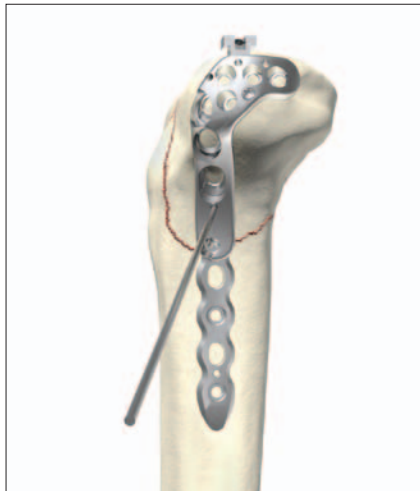


Fig. 6

The length is then measured using the Depth Gauge for Standard Screws (REF 702879) and an appropriate self-tapping 3.5mm Cortical Screw or a 4.0mm Cancellous Screw is then inserted using Screwdriver (REF 702841) (Fig. 8).

If inserting a cancellous screw, the near cortex must be pre-tapped using the Tap (REF 702805), and the Tear-drop Handle (REF 702428).

Any K-Wires in the shaft can be removed upon adequate screw fixation.

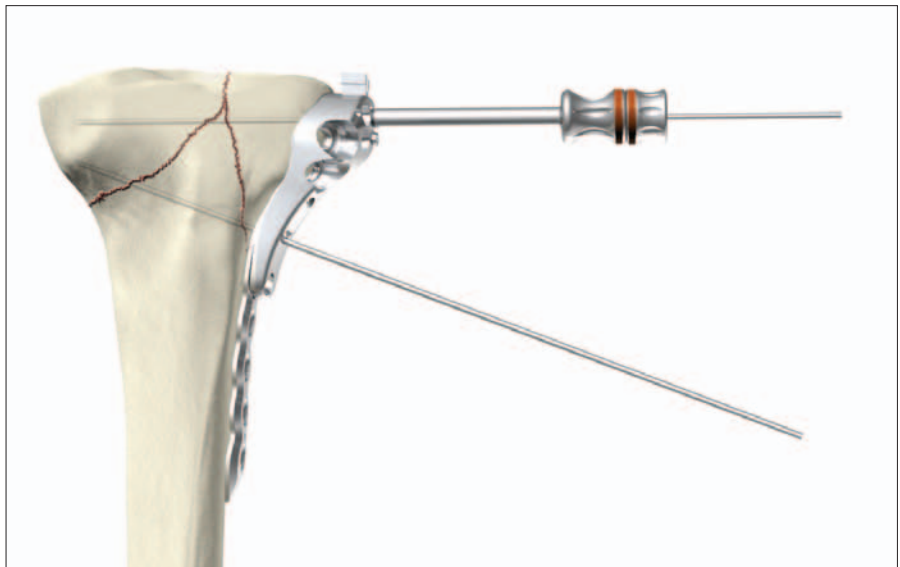


Fig. 7

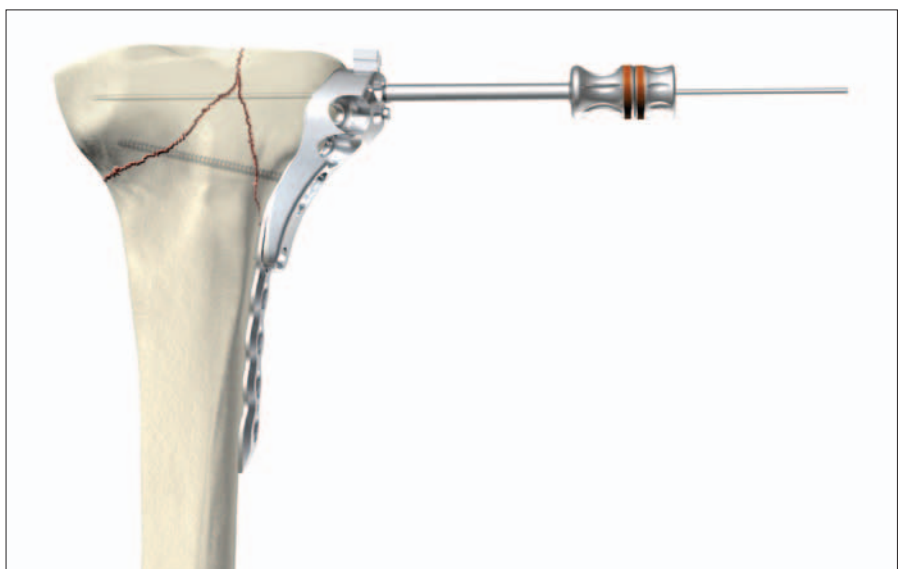


Fig. 8

Operative Technique

Step 6 – Primary Plate Fixation – Distal (Optional)

The distal end of the plate can now be secured. This can be achieved through one of four methods:

- A K-Wire inserted in the distal shaft K-Wire hole.
- A 3.5mm Cortex Screw using the standard technique.
- A 4.0mm Locking Screw in the pre-threaded locking holes or with a Locking Insert in the standard holes.
(see Step 8 – Shaft Fixation).
- The Temporary Plate Holder (REF 702776) in the last unthreaded shaft hole.

In addition to providing temporary fixation, the Plate Holder pushes the plate to the bone. Also, it has a self drilling, self tapping tip for quick insertion into cortical bone.

To help prevent thermal necrosis during the drilling stage, it is recommended that this device is inserted by hand.

Once the device has been inserted through the far cortex, the threaded outer sleeve/collet is turned clockwise until the plate is in contact with the bone (Fig. 9). The core diameter of this instrument is 2.4mm to allow a 3.5mm Cortical Screw to be subsequently inserted in the same shaft hole.

The Temporary Plate Holder can also be used for indirect reduction anywhere along the fracture site using the “Pull Reduction Method”.

Note:

A Locking Screw and Locking Insert should not be used in the hole where the Temporary Plate Holder is used.

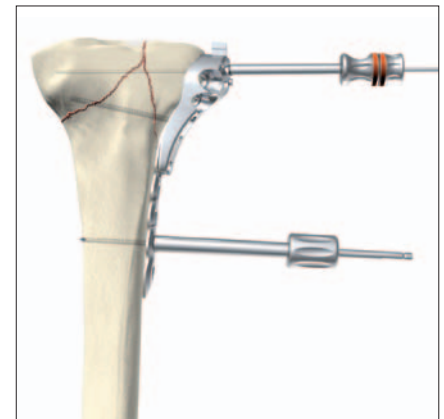


Fig. 9

Step 7 – Metaphyseal Locking

Locking Screws cannot act as Lag Screws. Should an interfragmentary compression effect be required, a 4.0mm Standard Cancellous Screw or a 3.5mm Standard Cortex Screw must first be placed in the unthreaded metaphyseal plate holes (Fig. 10) **prior** to the placement of any Locking Screws. Measure the length of the screw using the Depth Gauge for Standard Screws (REF 702879), and pre-tap the near cortex with the Tap (REF 702805) if a cancellous screw is used.

Consideration must also be taken when positioning this screw to ensure that it does not interfere with the given Locking Screw trajectories.

Fixation of the metaphyseal portion of the plate can be started using the preset K-Wire in the posterior locking hole as described in Step 5.

The length of the screw can be taken by using the K-Wire side of the Drill/K-Wire Measure Gauge (REF 702712) (See Locking Screw Measurement Guidelines on Page 8). Remove the K-Wire and K-Wire Sleeve leaving the Drill Sleeve in place.

A 3.1mm Drill (REF 702742) is then used to drill the core hole for the Locking Screw (Fig. 11).

Using Fluoroscopy, check the correct depth of the drill, and measure the length of the screw using the Depth Gauge for Locking Screws (REF 702884).



Fig. 10

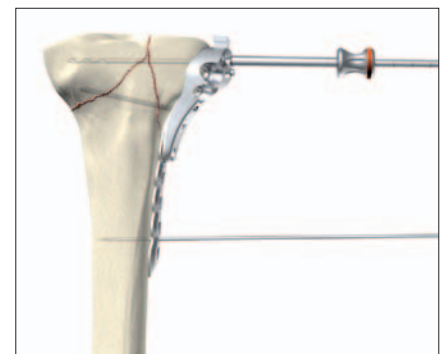


Fig. 11

Operative Technique

The Drill Sleeve should now be removed, and the correct length 4.0mm Locking Screw is inserted using the Screwdriver T15 (REF 702747) and Screw Holding Sleeve (REF 702732) (Fig. 12).

Locking Screws should initially be inserted manually to ensure proper alignment.

Note:

- Ensure that the screwdriver tip is fully seated in the screw head, but do not apply axial force during final tightening.
- If the Locking Screw thread does not immediately engage the plate thread, reverse the screw a few turns and re-insert the screw once it is properly aligned.

Final tightening of Locking Screws should always be performed manually using the Torque Limiting Attachment (REF 702750) together with the Solid Screwdriver T15 (REF 702753) and T-Handle (REF 702427) (Fig. 13). This helps to prevent over-tightening of Locking Screws, and also ensures that these Screws are tightened to a torque of 4.0Nm. The device will click when the torque reaches 4.0Nm.

Note:

The Torque Limiters require routine maintenance. Refer to the Instructions for Maintenance of Torque Limiters (REF V15020).

If inserting Locking Screws under power, make sure to use a low speed drill setting to avoid damage to the screw/plate interface and potential thermal necrosis. Perform final tightening by hand, as described above.

The remaining proximal Locking Screws are inserted following the same technique with or without the use of a K-Wire.

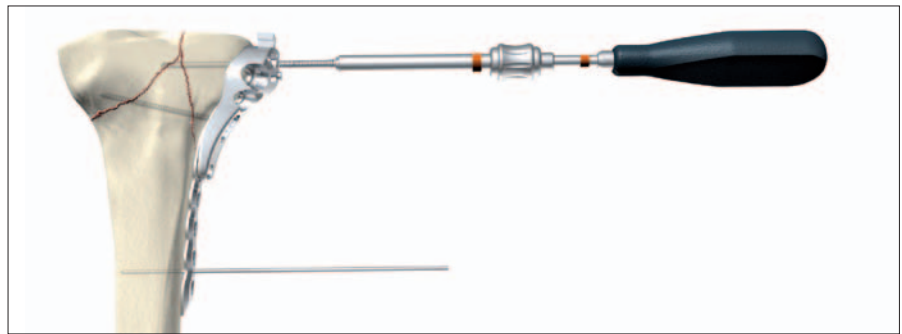


Fig. 12

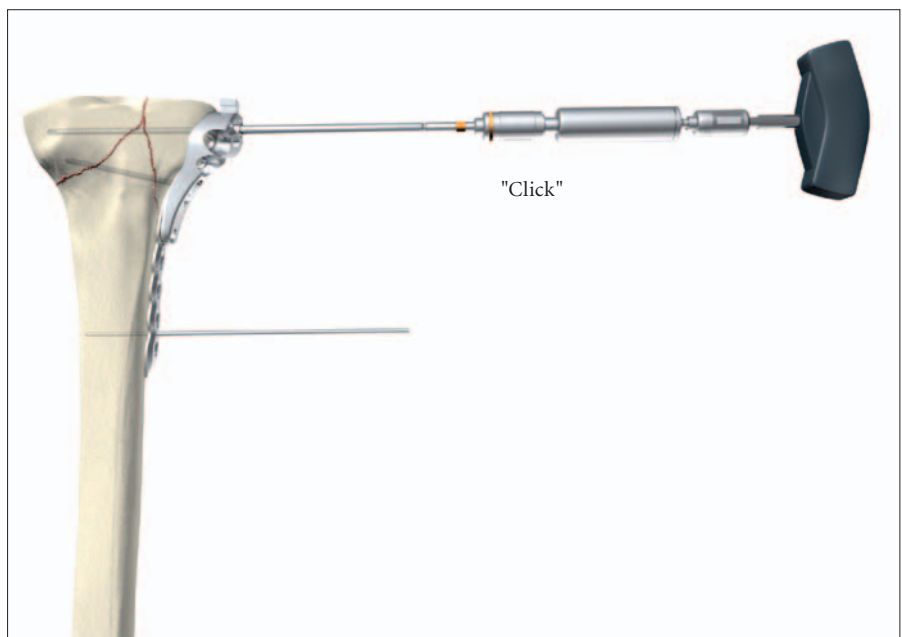
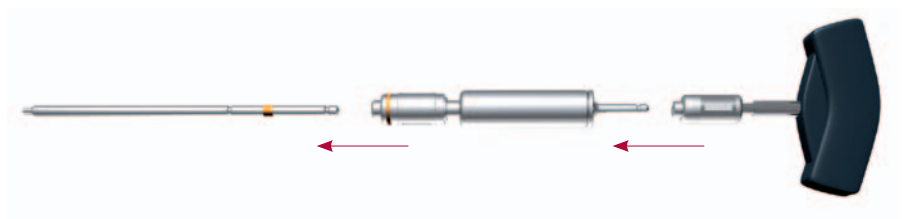


Fig. 13

Always use the Drill Sleeve (REF 702707) when drilling for locking holes.

To ensure maximum stability, it is recommended that all locking holes are filled with a Locking Screw of the appropriate length.

Operative Technique

Step 8 – Shaft Fixation

The shaft holes of this plate have been designed to accept either 3.5mm Standard Cortical Screws or 4.0mm Locking Screws. Locking Screws can be inserted in the predrilled locking holes or together with the corresponding Locking Inserts.

Note:

If a combination of Standard and Locking Screws is used in the shaft, the plate fixation should begin with Standard Cortical Screws prior to the Locking Screws. Always lag before you lock.



Locked Hole



70° Axial Angulation

14° Transverse Angulation

(Non-locked holes only)


Option 1 – Standard Screws

3.5mm Standard Cortical Screws can be placed in Neutral, Compression or Buttress positions as desired using the relevant Drill Guide and the standard technique.

These screws can also act as lag screws.

Note:

This is only possible in the non threaded holes.

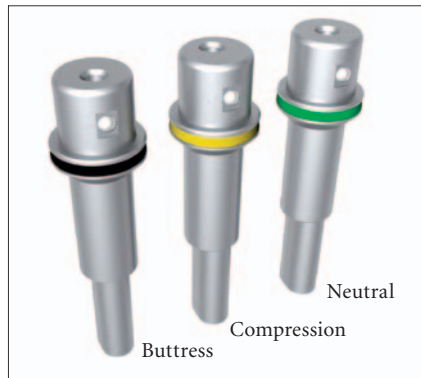

Buttress

Compression

Neutral



Operative Technique

Option 2 – Locking Screws

4.0mm Locking Screws can be placed in the threaded shaft holes or holes with pre-placed Locking Inserts.

Use the Drill Sleeve (REF 702707) to pre-drill the core hole for subsequent Locking Screw placement. The Drill Sleeve should be fully inserted into the thread of the locking hole or Locking Insert to ensure initial fixation of the Locking Insert into the plate. A 3.1mm Drill Bit (REF 702742) is used to drill through both cortices. (Fig. 14).

Note:

Avoid any angulation or excessive force on the drill, as this could dislodge the Locking Insert.

The screw measurement is then taken.

The appropriate sized Locking Screw is then inserted using the Solid Screwdriver T15 (REF 702753) and the Screw Holding Sleeve (REF 702732) together with the Torque Limiting Attachment (REF 702750) and the T-Handle (REF 702427).

Note:

Ensure that the screwdriver tip is fully seated in the screw head, but do not apply axial force during final tightening.

Maximum stability of the Locking Insert is achieved once the screw head is fully seated and tightened to 4.0Nm.

This procedure is repeated for all holes chosen for locked shaft fixation.

All provisional plate fixation devices (K-Wires, Temporary Plate Holder, etc) can now be removed.

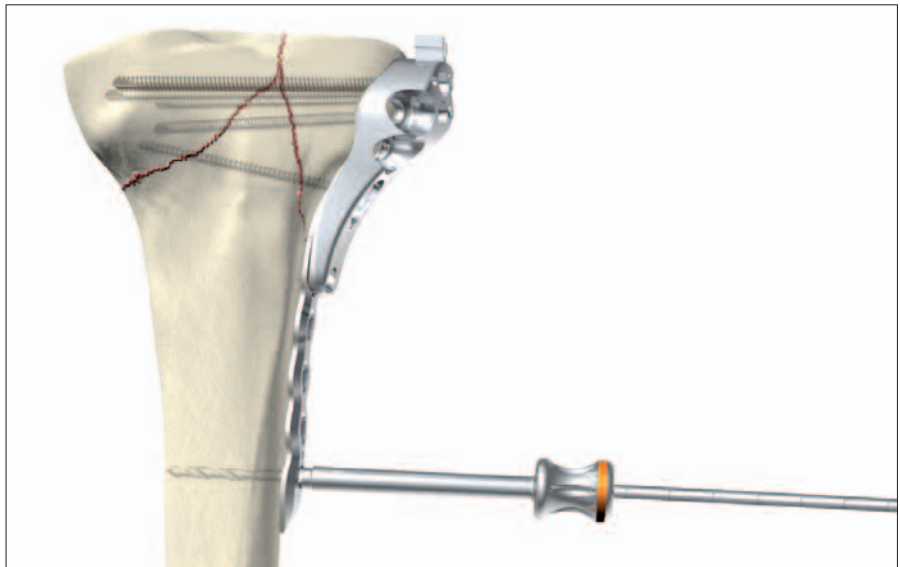


Fig. 14

Step 9 – Kick-Stand Screw Placement

The oblique "Kick-Stand" Locking Screw (Fig. 15) provides strong triangular fixation to the postero-medial metaphyseal fragment.

It should be the last screw in the metaphyseal portion of the plate.

It is advised that this screw is placed with the assistance of fluoroscopy to prevent joint penetration and impingement with the proximal Screws (See Step 7 for insertion guidelines). The Aiming Block should now be removed.

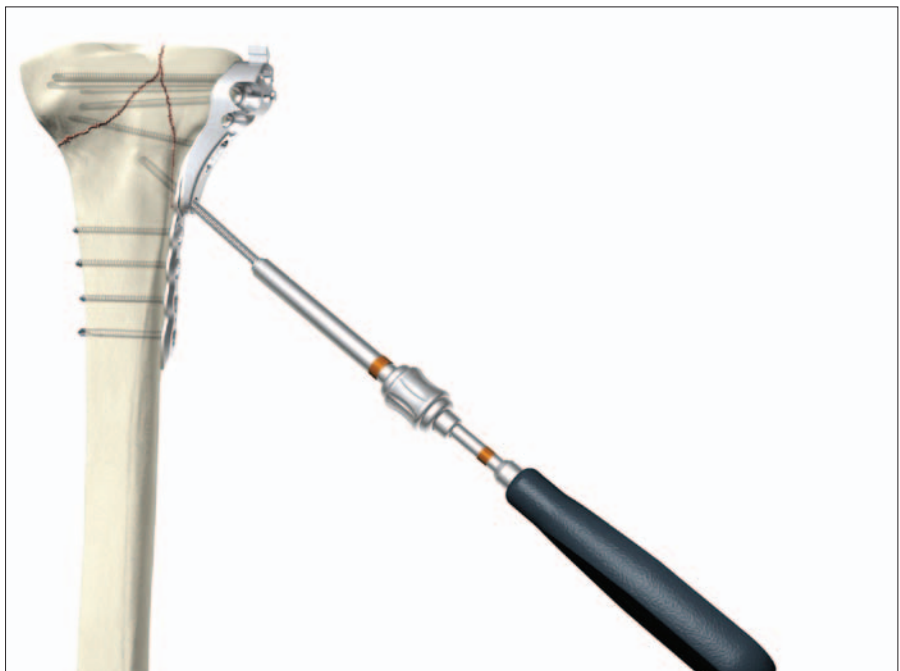


Fig. 15

Operative Technique

Sub-Muscular Insertion Technique

When implanting longer plates, a minimally invasive technique can be used.

The Soft Tissue Elevator (REF 702782) can be used to create a pathway for the implant (Fig. 16).

The plate has a special rounded and tapered end, which allows a smooth insertion under the soft tissue (Fig. 17).

Additionally, the Shaft Hole Locator can be used to help locate the shaft holes. Attach the appropriate side of

the Shaft Hole Locator (REF 702793) by sliding it over the top of the Handle until it seats in one of the grooves at an appropriate distance above the skin.

The slot and markings on the Shaft Hole Locator act as a guide to the respective holes in the plate.

A small stab incision can then be made through the slot to locate the hole selected for screw placement (Fig. 18). The Shaft Hole Locator can then be rotated out of the way or removed.



Fig. 16



Fig. 18



Fig. 17



Operative Technique

With the aid of the Soft Tissue Spreader (REF 702919) and Trocar (REF 702961) the skin can be opened to form a small window (Figures 19 & 20) through which either a Standard Screw or Locking Screw can be placed.

The Standard Percutaneous Drill Sleeve (REF 702709) or Neutral Percutaneous Drill Sleeve (REF 702957) in conjunction with the Drill Sleeve Handle (REF 702822) can be used to assist with drilling for Standard Screws.
Use a 2.5mm Drill Bit (REF 700355).

For Locking Screw insertion, use the threaded Drill Sleeve (REF 702707) together with the 3.1mm Drill Bit (REF 702742) to drill the core hole.

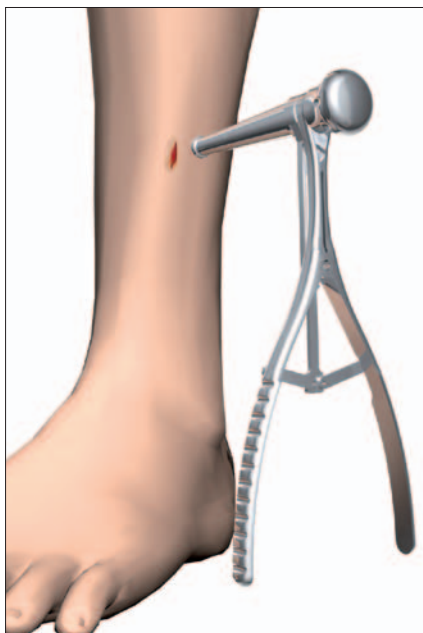


Fig. 19



Fig. 20

Final plate and screw positions are shown in Figures 21-23



Fig. 21



Fig. 22


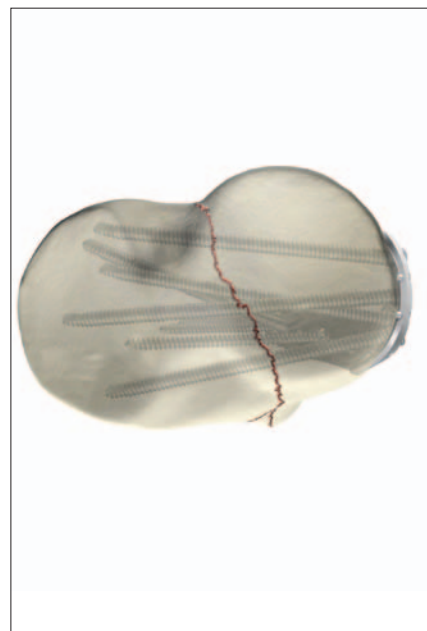


Fig. 23


Additional Tips

1. Always use the threaded Drill Sleeve when drilling for Locking Screws (threaded plate hole or Locking Insert).

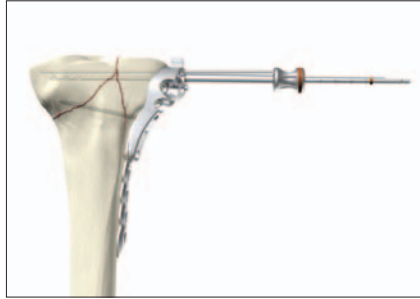


Free hand drilling will lead to a misalignment of the Screw and therefore result in screw jamming during insertion. It is essential, to drill the core hole in the correct trajectory to facilitate accurate insertion of the Locking Screws.

2. Always start inserting the screw manually to ensure proper alignment in the plate thread and the core hole. It is recommended to start inserting the screw using “the three finger technique” on the Teardrop handle. Avoid any angulations or excessive force on the screwdriver, as this could cross-thread the screw.

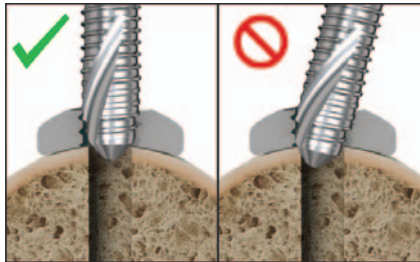

If the Locking Screw thread does not immediately engage the plate thread, reverse the screw a few turns and re-insert the screw once it is properly aligned.

3. If power insertion is selected after manual start (see above), use low speed only, **do not apply axial pressure**, and never “push” the screw through the plate!

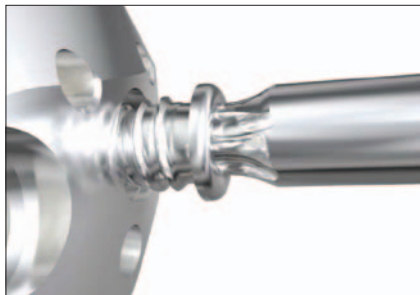


Allow the single, continuous threaded screw design to engage the plate and cut the thread in the bone on its own, as designed.

Power can negatively affect Screw insertion, if used improperly, damaging the screw/plate interface (screw jamming). This can lead to screw heads breaking or being stripped.

Again, if the Locking Screw does not advance, reverse the screw a few turns, and realign it before you start re-insertion.


Stop power insertion approximately 1cm before engaging the screw head in the plate.

4. It is advisable to **tap hard** (dense) **cortical bone** before inserting a Locking Screw. Use 4.0mm Tap (REF 702772).

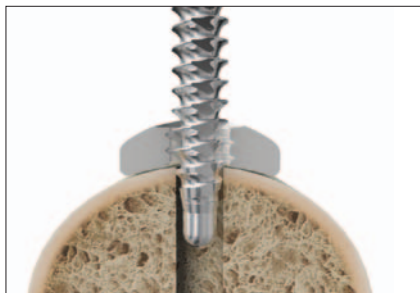

The spherical tip of the Tap precisely aligns the instrument in the predrilled core hole during thread cutting. This will facilitate subsequent screw placement.

5. Do not use power for final insertion of Locking Screws. It is imperative to engage the screw head into the plate using the Torque Limiting Attachment. Ensure that the screwdriver tip is fully seated in the screw head, but do not apply axial force during final tightening.

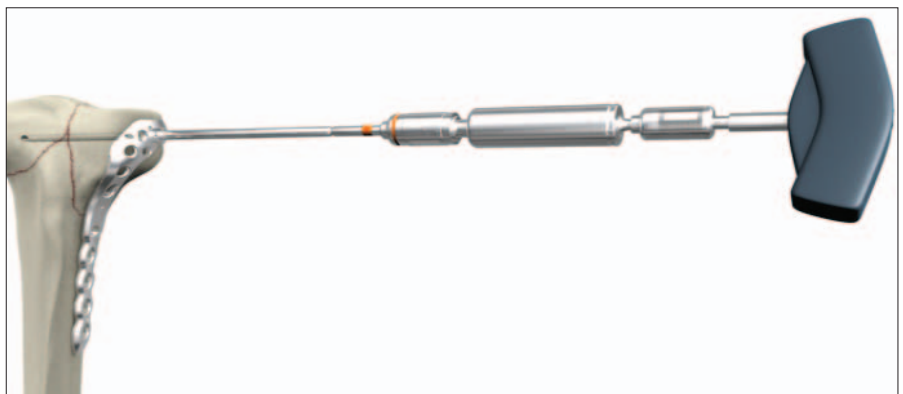

If the screw stops short of final position, back up a few turns and advance the screw again (with torque limiter on).

Ordering Information – Implants

PROXIMAL LATERAL TIBIA

Locking Screws 4.0mm

Standard Screws 3.5, 4.0mm



Left	Stainless Steel REF		Plate Length mm	Shaft Holes	Locking Holes Metaphyseal	Locking Holes Shaft
		Right				
	437302	437322	95	2	5	1
	437304	437324	121	4	5	2
	437306	437326	147	6	5	3
	437308	437328	173	8	5	4
	437310	437330	199	10	5	5
	437312	437332	225	12	5	6
	437314	437334	251	14	5	7

4.0MM LOCKING INSERT



Stainless Steel REF	System mm
370002	4.0

4.0MM CABLE PLUG



Stainless Steel REF	System mm
370004	4.0

Note:

For Sterile Implants,
add "S" to the REF.

Ordering Information – Implants

4.0MM LOCKING SCREW, SELF TAPPING

T15 Drive



Stainless Steel REF	Screw Length mm
371514	14
371516	16
371518	18
371520	20
371522	22
371524	24
371526	26
371528	28
371530	30
371532	32
371534	34
371536	36
371538	38
371540	40
371542	42
371544	44
371546	46
371548	48
371550	50
371555	55
371560	60
371565	65
371570	70
371575	75
371580	80
371585	85
371590	90
371595	95

4.0MM CANCELLOUS SCREW, PARTIAL THREAD


2.5mm Hex Drive



Stainless Steel REF	Screw Length mm
345514	14
345516	16
345518	18
345520	20
345522	22
345524	24
345526	26
345528	28
345530	30
345532	32
345534	34
345536	36
345538	38
345540	40
345545	45
345550	50
345555	55
345560	60
345565	65
345570	70
345575	75
345580	80
345585	85
345590	90
345595	95

3.5MM CORTICAL SCREW, SELF TAPPING

2.5mm Hex Drive

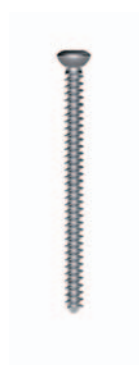

Stainless Steel REF	Screw Length mm
338614	14
338616	16
338618	18
338620	20
338622	22
338624	24
338626	26
338628	28
338630	30
338632	32
338634	34
338636	36
338638	38
338640	40
338642	42
338644	44
338646	46
338648	48
338650	50
338655	55
338660	60
338665	65
338670	70
338675	75
338680	80
338685	85
338690	90
338695	95

4.0MM CANCELLOUS SCREW, FULL THREAD

2.5mm Hex Drive



Stainless Steel REF	Screw Length mm
345414	14
345416	16
345418	18
345420	20
345422	22
345424	24
345426	26
345428	28
345430	30
345432	32
345434	34
345436	36
345438	38
345440	40
345445	45
345450	50
345455	55
345460	60
345465	65
345470	70
345475	75
345480	80
345485	85
345490	90
345495	95










Note:

For Sterile Implants,
add "S" to the REF.

Ordering Information – Instruments

	REF	Description
4.0mm Locking Instruments		
	702742	Drill Ø3.1mm × 204mm
	702772	Tap Ø4.0mm × 140mm
	702747	Screwdriver T15, L200mm
	702753	Solid Screwdriver Bit T15, L115mm
	702732	Screw Holding Sleeve
	702702	K-Wire Sleeve
	702707	Drill Sleeve
	702884	Direct Depth Gauge for Locking Screws
	702750	Universal Torque Limiter T15 / 4.0mm
	702762	Locking Insert Inserter 4.0mm
	702427	T-Handle Small, AO Fitting
	38111090	K-Wire (Trocac Point Steinmann Pin Ø2.0mm × 230mm)
	702767	Locking Insert Extractor
	702778	Handle for Plate Insertion
	702712	Drill/K-Wire Measure Gauge
	702776	Temporary Plate Holder
	702776-1	Spare Shaft for Temporary Plate Holder
	702919	Soft Tissue Spreader
	702961	Trocac (for Soft Tissue Spreader)
	702782	Soft Tissue Elevator
	702756	Bending Irons (×2)

Ordering Information – Instruments

	REF	Description
4.0mm Locking Instruments		
	702968	Locking Insert Forceps
	702671	Guide for Centering Pin
	702673	Centering Pin
	702675	Adapter for Centering Pin
	702729	Proximal Tibia, Aiming Block, Left
	702728	Proximal Tibia, Aiming Block, Right
	702720-2	Spare Set Screw for Tibia Aiming Block
	702793	Plate Trial/Shaft Hole Locator - Proximal Tibia
Optional Instruments		
	703616	Drill Ø3.1 × 204mm, flat Tip

Ordering Information – Instruments

REF	Description
SPS Standard Instruments	
700347	Drill Bit Ø2.5mm × 125mm, AO
700355	Drill Bit Ø2.5mm × 230mm, AO
700353	Drill Bit Ø3.5mm × 180mm, AO
702804	Tap Ø3.5mm × 180mm, AO
702805	Tap Ø4.0mm × 180mm, AO
702418	Drilling Guide Ø3.5/2.5mm
702822	Drill Sleeve Handle
702825	Drill Sleeve Ø2.5mm Neutral
702829	Drill Sleeve Ø2.5mm Compression
702831	Drill Sleeve Ø2.5mm Buttress
702709	Percutaneous Drill Sleeve Ø2.5mm
702957	Percutaneous Drill Sleeve Ø2.5mm Neutral
702879	Depth Gauge 0-150mm for Screws Ø3.5/4.0mm
702841	Screwdriver Hex 2.5mm for Standard Screws L200mm
702485	Solid Screwdriver Bit, Hex 2.5mm for Standard Screws L115mm
702490	Holding Sleeve for Screwdrivers For Screwheads: Ø6.0mm
702428	Tear Drop Handle, small, AO Fitting
900106	Screw Forceps
390164	K-Wires 1.6mm × 150mm (optional)
390192	K-Wires 2.0mm × 150mm



Other Instruments

702755	Torque Tester with Adapters
981081	X-Ray Template, Proximal Tibia

Cases and Trays

902955	Metal Base - Instruments
902929	Lid for Base - Instruments
902930	Instrument Tray 1 (Top)
902931	Instrument Tray 2 (Middle)
902963	Instrument Tray 3 (Bottom incl. Locking Insert Forceps)
902932	Screw Rack
902949	Metal Base - Screw Rack
902950	Metal Lid for Base - Screw Rack
902947	Metal Base - Implants
902971	Implant Tray - Proximal Lateral Tibia
902976	Lid for Implant Tray -Proximal Lateral Tibia
902958	Locking Insert Storage Box 4.0mm

Additional Information – HydroSet Injectable HA


Indications

HydroSet is a self-setting calcium phosphate cement indicated to fill bony voids or gaps of the skeletal system (i.e. extremities, craniofacial, spine, and pelvis). These defects may be surgically created or osseous defects created from traumatic injury to the bone. HydroSet is indicated only for bony voids or gaps that are not intrinsic to the stability of the bony structure.

HydroSet cured in situ provides an open void/gap filler than can augment provisional hardware (e.g. K-Wires, Plates, Screws) to help support bone fragments during the surgical procedure. The cured cement acts only as a temporary support media and is not intended to provide structural support during the healing process.




Tibial Plateau Void Filling

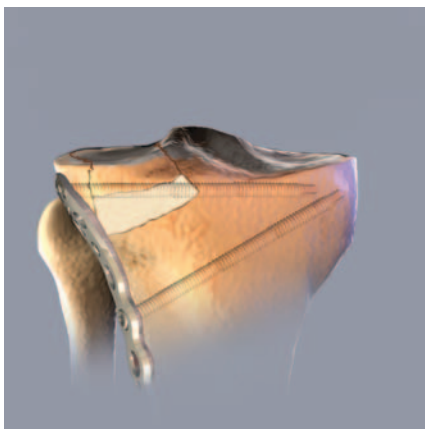

Note:

- Screw fixation must be provided by bone.
- For more detailed information refer to Literature No. 90-07900.

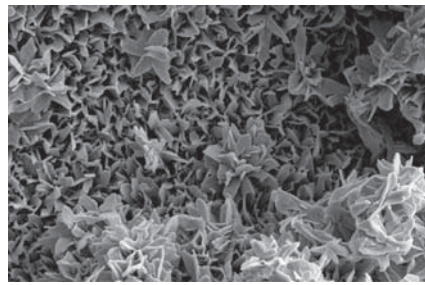

Scanning Electron Microscope image of HydroSet material crystalline microstructure at 15000x magnification

HydroSet is an injectable, sculptable and fast-setting bone substitute. HydroSet is a calcium phosphate cement that converts to hydroxyapatite, the principle mineral component of bone. The crystalline structure and porosity of HydroSet makes it an effective osteoconductive and osteointegrative material, with excellent biocompatibility and mechanical properties¹. HydroSet was specifically formulated to set in a wet field environment and exhibits outstanding wet-field characteristics². The chemical reaction that occurs as HydroSet hardens does not release heat that could be potentially damaging to the surrounding tissue. Once set, HydroSet can be drilled and tapped to augment provisional hardware placement during the surgical procedure. After implantation, the HydroSet is remodeled over time at a rate that is dependent on the size of the defect and the average age and general health of the patient.



CE 1275

Advantages

Injectable or Manual Implantation

HydroSet can be easily implanted via simple injection or manual application techniques for a variety of applications.

Fast Setting

HydroSet has been specifically designed to set quickly once implanted under normal physiological conditions, potentially minimizing procedure time.

Isothermic

HydroSet does not release any heat as it sets, preventing potential thermal injury.

Excellent Wet-Field Characteristics

HydroSet is chemically formulated to set in a wet field environment eliminating the need to meticulously dry the operative site prior to implantation².

Osteoconductive

The composition of hydroxyapatite closely match that of bone mineral thus imparting osteoconductive properties³.

Augmentation of Provisional Hardware during surgical procedure

HydroSet can be drilled and tapped to accommodate the placement of provisional hardware.

References

1. Chow, L, Takagi, L. A Natural Bone Cement – A Laboratory Novelty Led to the Development of Revolutionary New Biomaterials. J. Res. Natl. Stand. Technol. 106, 1029-1033 (2001).
2. 1808.E703. Wet field set penetration (Data on file at Stryker)
3. Dickson, K.F., et al. The Use of BoneSource Hydroxyapatite Cement for Traumatic Metaphyse

Ordering Information

REF	Description
397003	3cc HydroSet
397005	5cc HydroSet
397010	10cc HydroSet
397015	15cc HydroSet

Joint Replacements

Trauma, Extremities & Deformities

Craniomaxillofacial

Spine

Biologics

Surgical Products

Neuro & ENT

Interventional Spine

Navigation

Endoscopy

Communications

Imaging

Patient Care & Handling Equipment

EMS Equipment

Manufactured by:

Stryker Trauma AG
Bohnackerweg 1
CH - 2545 Selzach
Switzerland

www.osteosynthesis.stryker.com

This document is intended solely for the use of healthcare professionals. A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate a Stryker product. A surgeon must always refer to the package insert, product label and/or instructions for use, including the instructions for Cleaning and Sterilization (if applicable), before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: AxSOS, HydroSet, Stryker. All other trademarks are trademarks of their respective owners or holders.

The products listed above are CE marked.

Literature Number: **982299**
LOT **D4410**

Copyright © 2011 Stryker

