


T2 Recon Indication Metal Tray

Instrument Tray Layout


stryker®

Trauma

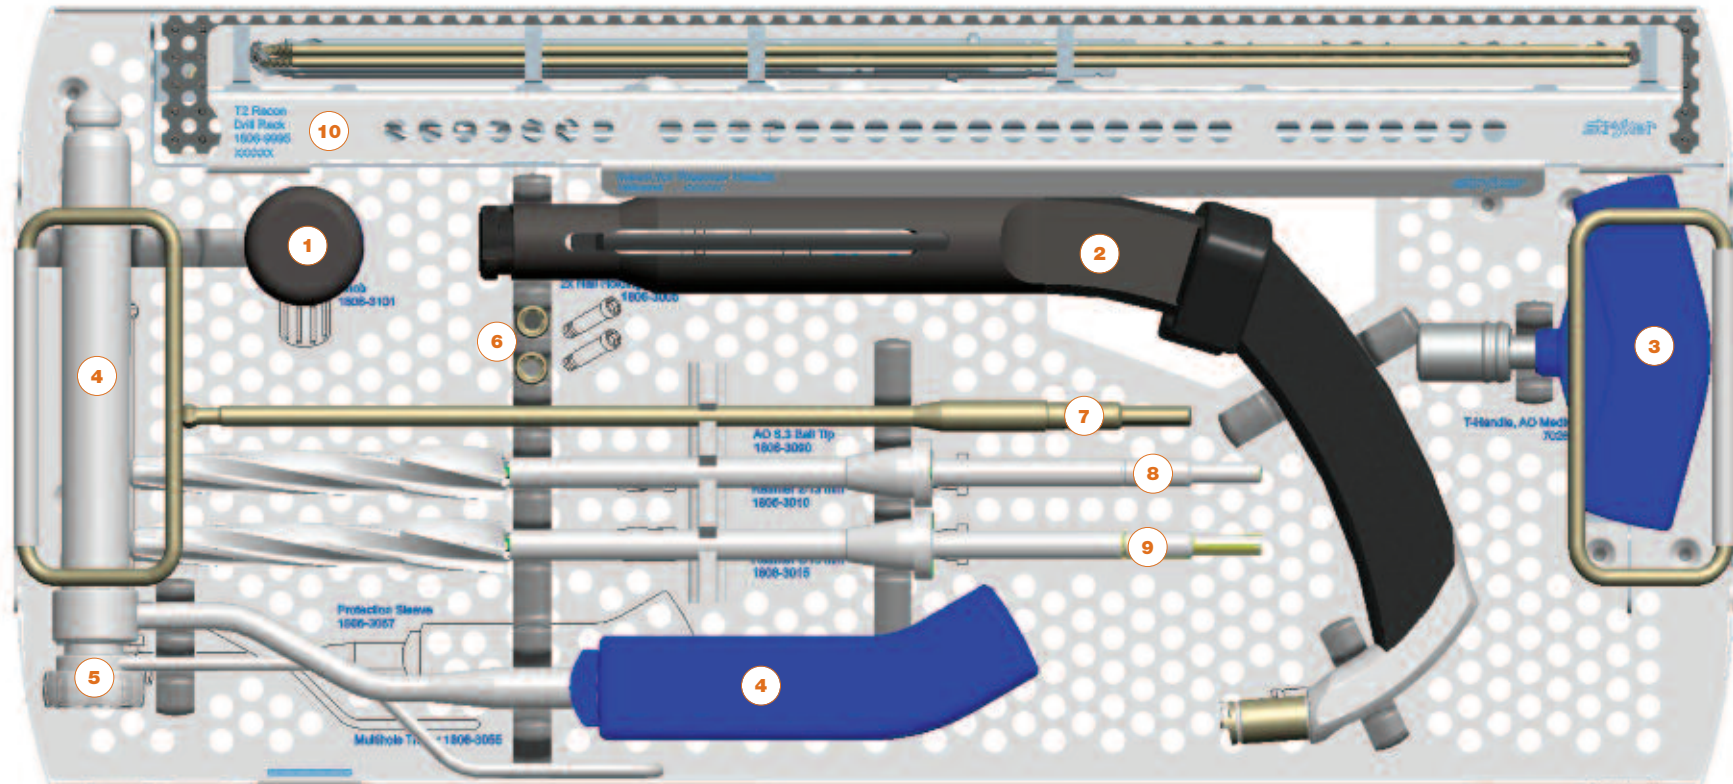

| Key | Item Description | Catalog No. |
|-----|---------------------------------|-------------|
| 1 | Knob | 1806-3101 |
| 2 | Target Device | 1806-3100 |
| 3 | T-Handle | 702628 |
| 4 | Protection Sleeve | 1806-3057 |
| 5 | Multihole Trocar | 1806-3055 |
| 6 | 2x Nail Holding Screws | 1806-3005 |
| 7 | Screwdriver Shaft, AO, Ball Tip | 1806-3090 |
| 8 | One Step Conical Reamer 13mm | 1806-3010 |
| 9 | One Step Conical Reamer 15mm | 1806-3015 |

| Key | Item Description | Catalog No. |
|-----|------------------|------------------------|
| 10 | Auxiliary Area | See Page 3 For Details |

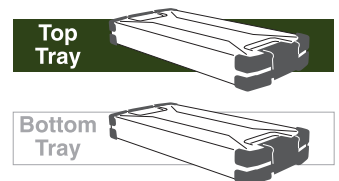


T2 Recon Indication Metal Tray

Instrument Tray Layout

stryker®

Trauma

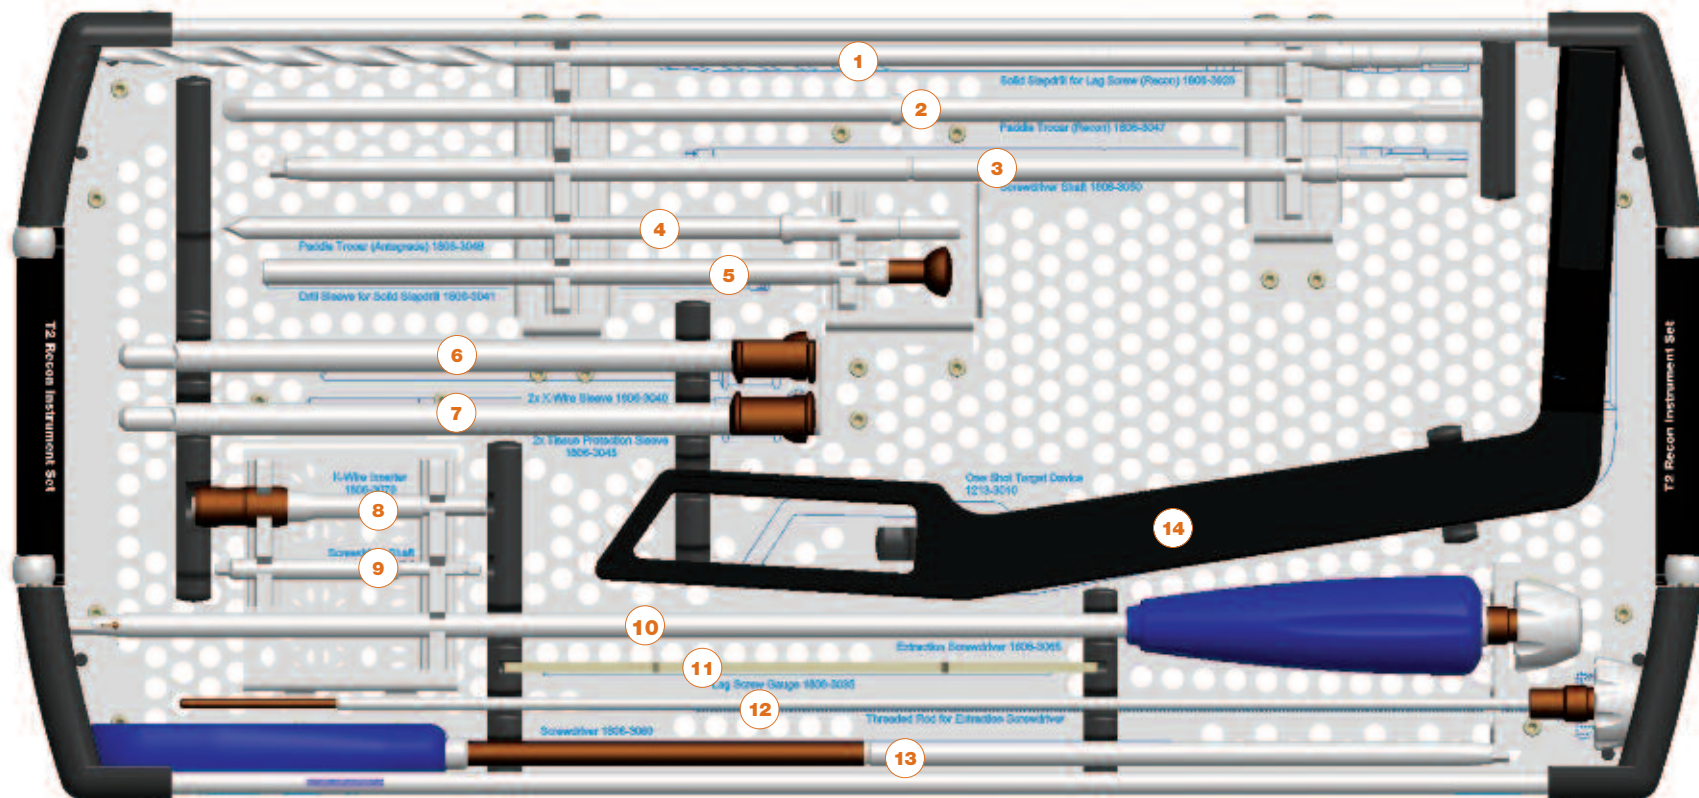

| Key | Item Description | Catalog No. |
|-----|--------------------------------------|--------------|
| 1 | Solid Stepdrill for Lag Screw, Recon | 1806-3026(S) |
| 2 | Paddle Trocar, Recon | 1806-3047 |
| 3 | Screwdriver Shaft | 1806-3050 |
| 4 | Paddle Trocar, Antegrade Mode | 1806-3048 |
| 5 | Drill Sleeve for Solid Stepdrill | 1806-3041 |
| 6 | 2x K-Wire Sleeve | 1806-3040 |
| 7 | 2x Tissue Protection Sleeve | 1806-3045 |
| 8 | K-Wire Inserter | 1806-3070 |
| 9 | Screwdriver Shaft, 3.5x | 1806-0292 |

| Key | Item Description | Catalog No. |
|-----|---|-------------|
| 10 | Extraction Screwdriver | 1806-3065 |
| 11 | Lag Screw Gauge | 1806-3035 |
| 12 | Threaded Rod for Extraction Screwdriver | 1806-3065 |
| 13 | Screwdriver, Recon | 1806-3060 |
| 14 | One Shot Device | 1213-3010 |




T2 Recon Indication Metal Tray

Instrument Tray Layout


stryker®

Trauma

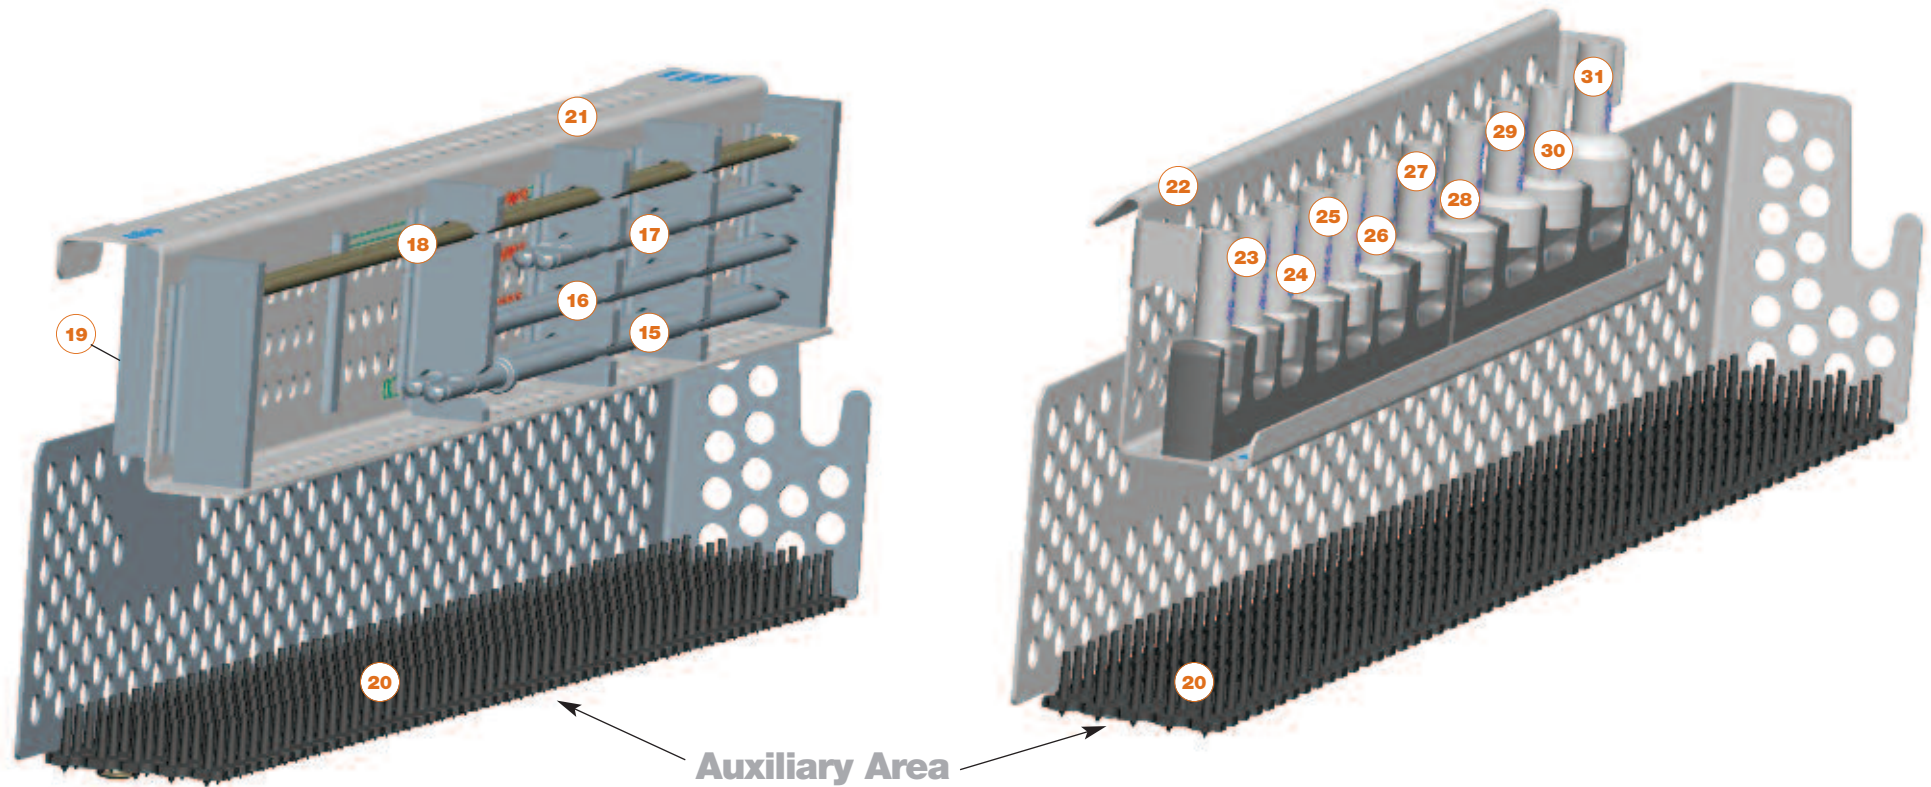

| Key | Item Description | Catalog No. |
|-----|------------------------------|-------------|
| 15 | 2x Drill 4.2 x 250mm Oblique | 1806-8018S |
| 16 | 2x Drill 4.2 x 230mm | 1806-4290S |
| 17 | 2x Drill 4.2 x 180mm | 1806-4270S |
| 18 | 2x K-Wire RECON | 1806-3031S |
| 19 | 2x Drill 4.2 x 340mm | 1806-4260S |
| 20 | Silicone Mat | 1806-9992 |
| 21 | Recon Drill Rack | 1806-9995 |

| Key | Item Description | Catalog No. |
|-----|--------------------------|-------------|
| 22 | BixCut Reamer Head Caddy | 1806-9996 |
| 23 | BixCut Reamer Head 9mm | 0226-3090 |
| 24 | BixCut Reamer Head 10mm | 0226-3100 |
| 25 | BixCut Reamer Head 11mm | 0226-3110 |
| 26 | BixCut Reamer Head 12mm | 0226-3120 |
| 27 | BixCut Reamer Head 13mm | 0226-3130 |
| 28 | BixCut Reamer Head 14mm | 0226-3140 |
| 29 | BixCut Reamer Head 15mm | 0226-3150 |
| 30 | BixCut Reamer Head 16mm | 0226-3160 |
| 31 | BixCut Reamer Head 17mm | 0226-3170 |

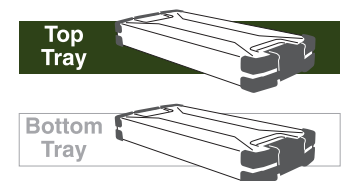



Joint Replacements

Trauma, Extremities & Deformities

Craniomaxillofacial

Spine

Biologics

Surgical Products

Neuro & ENT

Interventional Spine

Navigation

Endoscopy

Communications

Imaging

Patient Care & Handling Equipment

EMS Equipment

A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets.

Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: BixCut, Stryker, T2. All other trademarks are trademarks of their respective owners or holders.

Literature Number: LT2RI-TL
MS/GS 01/11

Copyright © 2011 Stryker
Printed in USA

325 Corporate Drive
Mahwah, NJ 07430
t: 201 831 5000

www.stryker.com