
## **Tray Layout Sheet – AxSOS 3 ORIF 4.0mm Instrument Tray**




		Description	Qty.			Description	Qty.
1	705004	Drill Sleeve 3.1mm Locking, Short	4	10	705019	Temporary Plate Fixator	2
2	705031	Drill Bit 3.1x216mm Locking, Short	2	11	705025	Drill Bit 2.5x216mm Non-locking, Short	2
3	705003	K-Wire Sleeve 2.0mm	2	12	705022	Drill Guide 2.5mm Non-locking	1
4	390192	K-Wire 2.0x150mm	10	13	702427	T-Handle , Small AO Coupling	1
5	705002	K-Wire with Drill Tip 2.0x234mm	10	14	702428	Teardrop Handle, Small AO Coupling	1
6	705012	Depth Gauge 0-120mm	1	15	702760	2.5Nm Torque Limiter	1
7	705013	Screw Scale	1	16	702782	Soft Tissue Elevator	1
8	705016	Screwdriver T15 (702747 optional)	1	17	705075	Drill Sleeve 3.1mm Locking, Medium	4
9	705015	Screwdriver Bit T15 (702753 optional)	2	18	705077	Drill Bit 3.1x238mm Locking, Medium	2




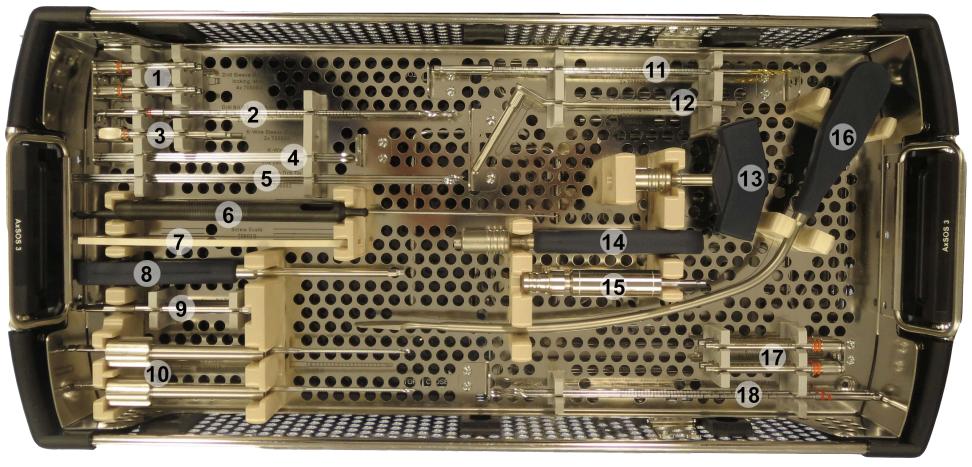

## **Tray Layout Sheet – AxSOS 3 ORIF 4.0mm Instrument Tray**

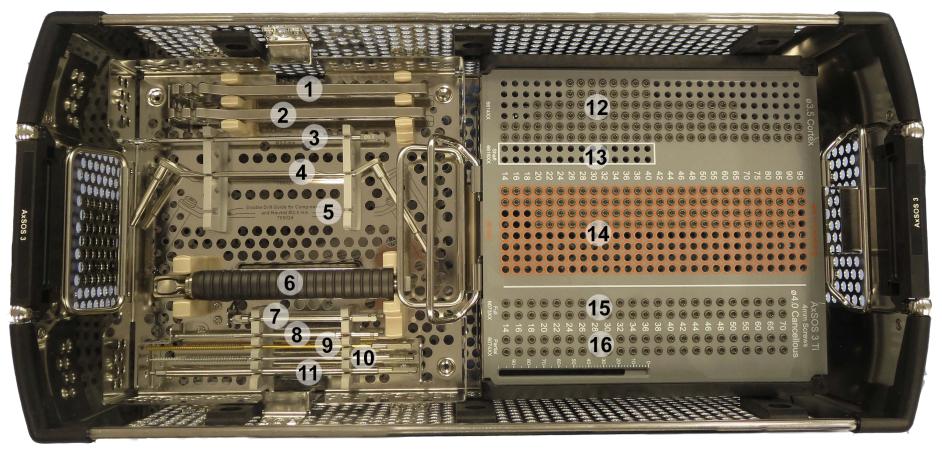

		Description	Qty.	Description			Qty.
1	705006	Bending Iron (Type 1)	1	9	702804	Tap, Cortical 3.5mm	1
2	705007	Bending Iron (Type 2)	1	10	702805	Tap, Cancellous 4.0mm	1
3	700353	Cortical Opener 3.5mm	1	11	703593	Screwdriver Bit HEX 2.5/4.3mm	1
4	705023	Double Drill Guide 3.5/2.5mm	1	12	661414 - 661495	3.5mm Cortex Screw, 14-95mm	
5	705024	Double Drill Guide 2.5mm (Compr/Nuetr)	1	13	661614 - 661640	3.5mm Cortex Shaft Screws (14-40mm special order)	
6	702778	Plate Insertion Handle	1	14	661014 - 661095	4mm Locking Screw, 14-95mm	
7	702811	Countersink	1	15	607314 - 607370	4mm Cancellous Screw, Full Thread, 14-70mm	
8	702772	Tap, Locking 4.0mm	1	16	607414 - 607470	4mm Cancellous Screws, Partial Thread, 14-70mm	
				I			



A surgeon must always rely on his or her own professional clinical judgment when deciding whether to use a particular product when treating a particular patient. Stryker does not dispense medical advice and recommends that surgeons be trained in the use of any particular product before using it in surgery.

The information presented is intended to demonstrate the breadth of Stryker product offerings. A surgeon must always refer to the package insert, product label and/or instructions for use before using any Stryker product. Products may not be available in all markets because product availability is subject to the regulatory and/or medical practices in individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: Stryker, AxSOS. All other trademarks are trademarks of their respective owners or holders.

Content ID: AXSOS-TLC-1, Rev 1, 11-2015 The products listed above are CE marked. Copyright © 2015 Stryker Manufacturer: Stryker GmbH Bohnackerweg 1 CH - 2545 Selzach Switzerland

www.stryker.com

